

Page 1 of 1

PATENT APPLICATION
RADIALLY EXPANSIBLE VESSEL SCAFFOLD
HAVING MODIFIED RADIOCAPACITY

Inventor:

ENRIQUE J. KLEIN, a citizen of the United States,
residing at 1686 Christina Drive
Los Altos, California 94024.

Assignee:

LEAP MEDICAL CORPORATION
1440 Koll Circle, Suite 103
San Jose, California 95112
A Delaware Corporation.

Status:

Small Entity

RADIALLY EXPANSIBLE VESSEL SCAFFOLD HAVING MODIFIED RADIOCAPACITY

CROSS-REFERENCES TO RELATED APPLICATIONS

The present invention is a continuation of U.S. Patent Application Serial
5 No. 08/968,319, filed on November 12, 1997, which was a continuation-in-part of
provisional U.S. Patent Application Serial No. 60/060,938, filed on October 23, 1997
(Attorney Docket No. 15509-5000) and PCT Application Serial No. PCT/US96/07942
filed on May 29, 1996 (Attorney Docket No. 15509-001700PC), which claims priority
from U.S. Patent Application 08/463,166, filed June 5, 1995 (Attorney Docket
10 No. 15509-001700), now U.S. Patent No. 5,593,442. The full disclosures of each of these
patents and patent applications are incorporated herein by reference.

BACKGROUND OF THE INVENTION

1. Field of the Invention

The present invention relates generally to the structure of radially
15 expansible luminal prostheses, including stents and grafts. More particularly, the present
invention relates to the provision of articulation structures for the construction of flexible
and pseudo-flexible prostheses and the provision of end structures for the construction of
atraumatically deliverable prostheses.

Luminal prostheses are provided for a variety of medical purposes. For
20 example, luminal stents can be placed in various body lumens, such as blood vessels, the
ureter, the urethra, biliary tract, and gastrointestinal tract, for maintaining patency.
Luminal stents are particularly useful for placement in pre-dilated atherosclerotic sites in
blood vessels. Luminal grafts can be placed in blood vessels to provide support in
diseased regions, such as aortic abdominal, and other aneurysms.

Both stent and graft prostheses must meet certain mechanical criteria to
25 function successfully. In particular, such prostheses should be at least partly flexible or
articulated (such as rigid sections that articulate relative to one another) over their lengths
so that they may be advanced through tortuous body lumens, such as those of the
coronary vasculature. In addition, the prostheses should preferably maintain their original
30 length or foreshorten minimally when the prostheses assume an expanded configuration.
Further such prostheses must have sufficient mechanical strength, particularly hoop

strength, in order to mechanically augment the luminal wall strength and thus assure lumen patency. The ability to meet these requirements is severely limited in the case of cylindrical endolumenal prostheses which are delivered in a radially constrained or collapsed configuration. Such prostheses must radially expand at a target site within the body lumen, so any adaptations which are intended to enhance flexibility will not interfere with the ability to radially expand or to maintain strength once expanded.

Prior lumenal prostheses often have structures which present a risk of injury as they are endolumenally delivered (i.e. tracked) to and/or released at a target site within a patient's body lumen. In particular, many vascular stents comprise a plurality of circumferentially connected and spaced-apart longitudinal elements which deform circumferentially as the stent is radially expanded. The Palmaz stent described in U.S. Patent Nos. 5,102,417 and 4,776,337, is typical of such stents. When these prostheses are flexed or articulated during delivery or tracking, these longitudinal elements of conventional prosthesis tend to create a phenomenon known as "fishscaling" which occurs when these elements distributed along the length of the prosthesis protrude outward from the surface of the prosthesis. Such stents exhibit poor "tracking" characteristics, where "tracking" is defined as the ability to pass smoothly through tortuous pathways. These protruding elements along the length of the prosthesis increase the likelihood that the prosthesis will dig into or otherwise engage the wall of the body lumen during delivery and even arrest the progress of the prosthesis and its delivery system to the diseased region (or target site). Additionally, a lesser-known phenomenon called "flaring" occurs when the longitudinal elements of the distal or proximal end of the prosthesis are bent outward to assume a crown-like configuration due to bending forces placed on these elements as the prosthesis passes through tortuous body passageways. Flaring can create the same deleterious effects as the previously described fishscaling phenomenon, injuring or traumatizing the blood vessel wall as the prosthesis is delivered or tracked within the blood vessel.

A separate problem in stent construction and deployment relates to the ability to detect the stent fluoroscopically during the deployment procedure. Stainless steel, the most common stent material, is generally radiolucent, i.e. it is minimally visible under x-rays and permits fluoroscopic examination therethrough. Advantageously, such stents do not interfere with subsequent fluoroscopic examination of the treated region of the body lumen, such as six-month-followup examinations. They are, however, much more difficult to accurately position within the lumen due to their radiolucency. To

increase radiopacity, these prostheses may be manufactured from radiopaque materials such as tantalum, platinum, or nickel titanium (NiTi). Alternatively, the entire prosthesis may be plated or coated with a uniform layer of radiopaque material to improve prosthesis visualization as disclosed in commonly assigned, co-pending U.S. Patent application Serial No. 08/691,661, filed August 2, 1996 (Attorney Docket No. 15509-003900), the complete disclosure of which is incorporated herein by reference. Although these methods address the issue of radiopacity, uniform layers of such materials or prostheses made entirely of such materials typically improve radiopacity at the cost of reduced visibility of tissue inside the prosthesis.

For these reasons, it would be desirable to provide improved stents and other luminal prostheses. In particular, it would be desirable to provide improved luminal prostheses and methods for their endolumenal placement, where the prostheses can be delivered or tracked to a target site within a body lumen without traumatically engaging the walls of the body lumen. Preferably, the prostheses will have elements which minimize "fishscaling" with its concomitant risk of injury or even retention within the body lumen. Such prostheses may also be provided with minimally traumatic end rings in order to reduce the risk of luminal injury as the prostheses is both delivered and radially expanded within the body lumen. Optionally, the ends of the prostheses may incorporate stiffening elements which reduce the occurrence of prosthesis flaring or trumpeting during tracking through tortuous body lumens. Additionally, the prostheses will be radially expansible at the target location, and will preferably retain both their cylindrical configuration and flexibility or ability to articulate after expansion. Such prostheses should further have sufficient hoop strength and other mechanical characteristics so that they may effectively function as stents in maintaining luminal patency and/or grafts in enhancing luminal wall strength. To more precisely direct scaffolding force at a diseased site, the prosthesis may have specific expanded configurations. Furthermore, it would be desirable to provide improved prostheses having radiopacity characteristics which permit visualization of the prosthesis both during tracking and deployment as well as visualization of tissue within the lumen during subsequent angiographic followup after deployment. The present invention will provide at least some of the desired improvements.

2. Description of the Background Art

Vascular stents comprising multiple segments joined by axial hinge structures are described in U.S. Patent Nos. 5,195,984; 5,104,404; and 5,102,417 and European Patent Publication EP 540 290. Other stent structures are described in U.S. patent 5,282,824, European Patent Publication EP 481 365; and Canadian Patent Publication 2,079,944. U.S. Patent No. 4,776,337 describes the Palmaz stent which consists of multiple longitudinal box elements joined to each other by short circumferentially oriented tabs and usually having at least two such sections joined longitudinally by a single short beam as shown in U.S. Patent No. 5,195,984.

SUMMARY OF THE INVENTION

The present invention provides improved prostheses and methods for their endolumenal placement within body lumens, particularly blood vessels. The prostheses may be in the form of stents, intended for maintaining lumenal patency, or may be in the form of grafts, intended for protecting or enhancing the strength of the lumenal wall. The prostheses of the present invention will be radially expandible, either by the application of an internal force to expand a minimally resilient (usually malleable) prosthesis structure or by release of radial constraint from a resilient prosthesis structure (self-expanding).

In a first aspect of the present invention, the prosthesis comprises a plurality of radially expandible unit segments, such as rings, having a plurality of beams connecting axially remote points on adjacent unit segments, and a plurality of compliant elements referred to hereinafter as expansion joints connecting axially proximate points on adjacent unit segments. The beams are usually aligned axially and maintain the remote points at a fixed distance at all times including when the prosthesis is radially expanded. The expansion joints, in contrast, allow for relative movement of the proximate points during bending, expansion, or any other deformation of the prosthesis. The expansion joint may have any convenient geometry, such as an "S" shape, a "Z" shape, a serpentine pattern, a zig-zag pattern, or the like. Thus, the expansion joints will provide a compliant, flexible connection of the proximate points on the unit segments to reduce or prevent protrusion or "fishscaling" of these points as the prosthesis is delivered through a tortuous path or deployed (expanded) at a curved target site.

To create the tracking and expansion characteristics desired in the prosthesis, the beams and expansion joints may be positioned in particular patterns between each unit segment. For example, although adjacent unit segments of the

prosthesis may be coupled by both expansion joints and beams, they are preferably joined by only one beam and some number of expansion joints. Having only one beam balances the benefits of length compensation and prosthesis flexibility. Beams of the prosthesis are preferably positioned in a "laddered" configuration where the sequence of

5 longitudinal beams is circumferentially and longitudinally staggered, typically with a predetermined amount of longitudinal overlap between the beams when in the unexpanded configuration. The amount of overlap may be about one-third the length of each beam or more preferably one-half the length of each beam. In certain embodiments, beams may also have a weakened midportion of lesser width or lesser thickness than the

10 remainder of the beam to increase transverse flexibility of the prosthesis. The expansion joints may also be weakened to maximize flexibility and minimize interference with the ability of the prosthesis to track. Typically, weakened expansion joints have smaller width or smaller thickness than the longitudinal struts in the unit segments.

In a second aspect of the present invention, the prosthesis may include

15 elements to increase radial stiffness both when unexpanded and when expanded, such as an end segment requiring a greater radial expansion force than another segment in the middle of the prosthesis. In one embodiment, the end segment is a serpentine ring having longitudinal struts of shorter length than the longitudinal struts of segments in the middle of the cylindrical frame. Alternatively, the end rings could have increased stiffness by

20 using hinges of increased width or thickness between each longitudinal portion or strut, as disclosed in commonly assigned, co-pending U.S. Patent application Serial No. 08/691,661, filed August 2, 1996 (Attorney Docket No. 15509-003900), the complete disclosure of which has been previously incorporated herein. Increased radial stiffness at the ends of the prosthesis, such as through struts of shorter lengths or box structures with

25 unequal strut lengths, tends to reduce flaring or trumpeting of these ends which may occur during tracking through tortuous passageways. A still further improvement for reducing prosthesis flaring or trumpeting involves using a radially stiffened end segment that is hinged by a long beam to an adjacent segment. The single beam provides articulation between the segments and thus reduces the load placed on the struts in the

30 end segments. Additionally, a prosthesis can be mounted on an inflation member such as a balloon which can shape the expanded prosthesis into a noncylindrical shape. For example, the prosthesis may be expanded into a tapered configuration to provide improved fit and scaffolding in body lumens which have conical configurations. The ability of the inflation member, such as a noncylindrical balloon, to expand a prosthesis

into a shape that better conforms to the luminal geometry may also be enhanced by having unit segments of various radial stiffnesses, such as having a stiffness gradient from one segment to the next, or other nonuniform stiffnesses along the length of the prosthesis.

5 In a third aspect, a system according to the present invention includes a cylindrical frame forming a prosthesis having a plurality of radially expandible unit segments, a longitudinal length, a distal end and a proximal end. The frame is preferably mounted over an expandible cylindrical section of an inflation member such as a balloon. In this third aspect, the expandible cylindrical section has the same length as the length of
10 the cylindrical frame. Advantageously, this minimizes expansion of the balloon beyond the ends of the prosthesis which may do dissectogenic damage, particularly to the distal the body lumen in which the system is delivered. The inflation section of the balloon is preferably no more than about 1 mm longer from each end of the typically cylindrical frame, more preferably about the same length as the cylindrical frame. The present
15 invention also provides a kit with instructions for use describing a method for mounting a prosthesis over such a matching length balloon together with a mounting tool.

 In a fourth aspect, a prosthesis according to the present invention may have a coating of radiopaque material such as gold covering at least the entire outer surface of the prosthesis. The coating will preferably have areas of a first desired
20 thickness and other areas of a second desired thickness. In one embodiment, the ends of the prosthesis have a coating of 0.0006 inches of gold while the remainder of the prosthesis, typically the middle area, has a coating of 0.0003 inches. In another embodiment, a prosthesis may be created using the method of the present invention to create ends having a coating of 0.0006 inches of gold while the middle area has no
25 coating at all. Advantageously, a prosthesis having different thicknesses of radiopaque material added to a radiolucent prosthesis will facilitate the accurate positioning of the prosthesis in the lumen while also allowing for tissue examination following the expansion of the prosthesis and during angiographic followup.

 In a further aspect, the present invention provides a method for reinforcing
30 the wall of a body lumen by introducing a prosthesis, having the proximal points of the unit segments constrained by expansion joints and the remote points of adjacent units segments joined preferably by a single beam, to a target site within the body lumen and radially expanding the prosthesis once the target site is reached. The prosthesis may be expanded by applying an expansive force, such as that supplied by a balloon catheter, or

alternatively, the prosthesis may be released from a radial constraint at the target site. Alternatively, the method of the present invention may comprise delivering and then expanding a prosthesis having radially constrained or limited ends to reduce the likelihood of prosthesis flaring or trumpeting during delivery or tracking through tortuous body passageways.

A further understanding of the nature and advantages of the invention may be realized by reference to the remaining portions of the specification and the drawings.

BRIEF DESCRIPTION OF THE DRAWINGS

Fig. 1 shows a longitudinal side view of a prosthesis according to the present invention.

Fig. 2 is a “rolled out” view of a first exemplary embodiment of a prosthesis of the present invention.

Fig. 3A shows a longitudinal side view of portions of a prosthesis using box structures.

Fig. 3B shows a longitudinal side view of portions of a prosthesis using zig-zag structures.

Fig. 3C shows a prior art prosthesis in a curved configuration exhibiting “fishscaling.”

Fig. 3D shows the prosthesis of Fig. 1 in a curved configuration.

Figs. 4A-4C show a side view of an expansion joint according to the present invention.

Figs. 5-7 illustrate a side view of alternative embodiments of an expansion joint of the present invention.

Figs. 8A-8D show length compensation effects for beams and box structures used in the present invention.

Fig. 9 is a perspective view of a portion of a serpentine ring.

Fig. 10A depicts a prior art stent displaying flared ends due to tracking.

Fig. 10B shows a prosthesis of the present invention having radially stiffer end rings.

Fig. 11 is a “rolled out” view of a second exemplary embodiment of a prosthesis of the present invention.

Fig. 12 shows an alternate embodiment of a device for minimizing flaring in a prosthesis.

Fig. 13 shows a prosthesis of the present invention mounted on a balloon of a catheter.

Fig. 14 shows a catheter/prosthesis assembly of Fig. 6 being endovascularly delivered or tracked to a target site in a body lumen.

Figs. 15A-15D shows the catheter/prosthesis system of Figs. 13 and 14 being delivered, expanded, and secured in a body lumen.

Figs. 16A-16C are cross-sectional views of the expansion of a balloon and prosthesis resulting in dissectogenic bulbous ends.

Figs. 17A-17C are cross-sectional views of the expansion of a length matched balloon and prosthesis of Figs. 13 and 14.

Figs. 18A-18C illustrate a method for mounting a prosthesis onto an expansible inflation member.

Fig. 19 shows a kit according to the present invention.

Figs. 20A-20F show prostheses with various unit segment configurations.

Figs. 21A-21E depict cross-sectional views of a prosthesis being covered with a layer of radiopaque material having selective thicknesses according to the present invention.

Figs. 22A-22C show cross-sectional views of a prosthesis being covered by a method for depositing a layer of radiopaque material having selective thicknesses according to the present invention.

DESCRIPTION OF THE SPECIFIC EMBODIMENTS

I. Introduction

The present invention provides devices and methods for the endolumenal placement of prostheses, particularly within the vascular system for the treatment of cardiovascular disease, such as vascular stenoses, dissections, aneurysms, and the like. The apparatus and methods, however, are also useful for placement in other body lumens, such as the ureter, urethra, biliary tract, gastrointestinal tract and the like, for the treatment of other conditions which may benefit from the introduction of a reinforcing or protective structure within the body lumen. The prostheses will be placed endolumenally. As used herein, "endolumenally" will mean placement through a body opening or by percutaneous or cutdown procedures, wherein the prosthesis is translumenally advanced through the body lumen from a remote location to a target site in the lumen. In vascular procedures, the prostheses will typically be introduced "endovascularly" using a catheter

over a guidewire under fluoroscopic guidance. The catheters and guidewires may be introduced through conventional access sites to the vascular system, such as through the femoral artery, or brachial, subclavian or radial arteries, for access to the coronary arteries.

5 A luminal prosthesis according to the present invention will comprise usually at least two radially expansible, usually cylindrical, body or unit segments. By “radially expansible,” it is meant that the segment can be converted from a small diameter configuration (used for endolumenal placement) to a radially expanded, usually
10 cylindrical, configuration which is achieved when the prosthesis is implanted at the desired target site. The prosthesis may be minimally resilient, e.g., malleable, thus requiring the application of an internal force to expand and set it at the target site. Typically, the expansive force can be provided by a balloon, such as the balloon of an angioplasty catheter for vascular procedures. As will be described below, the present invention provides atraumatic connections between successive unit segments which are
15 particularly useful to prevent “fishscaling” in prosthesis which are not protected by sheaths during delivery. Alternatively, the prosthesis can be self-expanding. Such self-expanding structures are provided by utilizing a resilient material, such as a tempered stainless steel or a superelastic alloy such as an NiTi alloy, and forming the body segment so that it possesses its desired, radially-expanded diameter when it is unconstrained, i.e.
20 released from the radially constraining forces of a sheath. In order to remain anchored in the body lumen, the prosthesis will remain partially constrained by the lumen. The self-expanding prosthesis can be tracked and delivered in its radially constrained configuration, e.g. by placing the prosthesis within a delivery sheath or tube and removing the sheath at the target site.

25 The dimensions of the luminal prosthesis will depend on its intended use. Typically, the prosthesis will have a length in the range from about 5 mm to 100 mm, usually being from about 8 mm to 50 mm, for vascular applications. The small (radially collapsed) diameter of cylindrical prostheses will usually be in the range from about 1 mm to 10 mm, more usually being in the range from 1.5 mm to 6 mm for vascular
30 applications. The expanded diameter will usually be in the range from about 2 mm to 50 mm, preferably being in the range from about 2.5 mm to 30 mm for vascular applications.

The body or unit segments may be formed from conventional materials used for body lumen stents and grafts, typically being formed from malleable metals, such as 300 series stainless steel, or from resilient metals, such as shape memory alloys,

e.g. NiTi alloys, spring steel, and the like. It is possible that the body segments could be formed from combinations of these metals, or combinations of these types of metals and other non-metallic materials. Additional structures for the body or unit segments of the present invention are illustrated in U.S. Patent Nos. 5,195,417; 5,102,417; and 4,776,337, the full disclosures of which are incorporated herein by reference.

The present invention provides improvements over conventional stents by including both beams and compliant members, preferably nonradially protruding expansion joints, in the design of the prosthesis to minimize longitudinal foreshortening during radial expansion and to maintain a generally smooth outer surface on the prosthesis during delivery. The beams and expansion joints connect together a plurality of unit segments, such as rings with serpentine and/or box structures, and hold the segments at a substantially fixed distance apart from one another. The expansion joints are preferably connected between protruding elements of the unit segments and prevent these protrusions from engaging the wall of the body lumen as the prosthesis is traversed through in the body lumen. The expansion joint is designed to accommodate the flexing of the prosthesis that occurs when tracking the device through tortuous passageways in the body.

The present invention may further include unit segments such as radial rings having increased radial stiffness on the distal and proximal ends of the prosthesis. Radial expansion as well as compression stiffness may be increased by shortening the length of longitudinal struts in the ring. These longitudinally shorter unit segments, which may take the form of rings with box structures or serpentine structures, are more resistant to radial expansion than rings having longer struts. Alternatively, segments may be made stiffer by adjusting the hinges connecting the struts together. Whether these stiffer segments are directly connected to the adjacent unit segments or connected by long single beams, these structures minimize flaring or trumpeting of the ends of the prosthesis. Flaring or trumpeting of the prosthesis occurs due to its transverse stiffness which resists the bending and curving of the prosthesis mounted on its delivery catheter during tracking through tortuous pathways. The flaring or trumpeting is undesirable as it will likely cause the prosthesis to engage the body lumen wall and either create trauma to the wall or arrest the delivery of the prosthesis to a target site. Additionally, the prosthesis may be mounted on an expansible inflation member, such as a balloon, having a typically cylindrical inflation section of about the same length as the catheter to reduce especially distal dissectogenic expansion of the balloon. The prosthesis may also be

mounted on expansible inflation members with shaped expanded configurations, such a single or multiple taper, to match the prosthesis to the contour of the body lumen or to direct dilatation force of the prosthesis at a target site, such as the ostium of a body lumen.

5 Still further, the present invention may improve over conventional prostheses by having a coating of radiopaque material having selective thicknesses covering at least parts of the surface of the prosthesis. Advantageously, this allows the radiopacity of the prosthesis to be customized to create, for example, more radiolucent midsections for increased visualization of treated tissue inside the prosthesis while having
10 more radiopaque end sections for facilitating positioning one and juxtaposing/overlapping more than one of the prostheses in a body lumen. These coatings of radiopaque materials may be applied by using selective electroplating or other processes such as dipping or sputtering.

15 While the prostheses of the present invention will preferably include beams/expansion joints, radially stiffer segments, and selective radiopaque marking schemes as described, it will be appreciated that each of these aspects of the present invention may be employed by itself or in other combinations to provide an improved prosthesis.

20 II. Embodiments of the Prosthesis

Referring now to Fig. 1, a radially expansible luminal prosthesis 10 generally comprises a frame 20 formed from a plurality of radially expansible unit segments 22. Although the final shape of the prosthesis 10 will generally be cylindrical, it should be appreciated that the prosthesis may also be conformable to non-cylindrical cross-sectional lumens and may also be conformable to transversely curved lumens. In a
25 first exemplary embodiment of Fig. 2, the frame 20 is formed from a plurality of longitudinally adjacent unit segments 22 connected to one another by a plurality of beams 24 and expansion joints 26. The frame 20 is typically defined as having a midsection 27 which comprises those segments 22 which are not on the longitudinal ends of the frame.

A. *Unit Segments*

30 The radially expansible unit segment 22 is the building block from which the frame 20 is formed. Unit segment 22 is preferably formed in the shape of a single, elongate element patterned in a serpentine or “undulating” configuration. It should be noted, however, that a variety of structures incorporating members such as box 30 or zig-

zag shapes 32 shown in Figs. 2, 3A ,and 3B may be used so long as the resulting unit segments 22 are capable of producing the desired radial expansion of luminal prosthesis 10. Box 30 typically has sets of longitudinal struts 31 and 33 of unequal lengths. The unit segments 22 typically retain a “zig-zag”, diamond, or other pattern even after radial expansion to provide adequate support or scaffolding for the vessel wall between consecutive segments and to inhibit localized hyperplasia. Conveniently, the entire prosthesis 10, including the unit segments, beams, and expansion joints can be formed by laser cutting, electric discharge machining, or photochemical etching of thin-wall tubular (i.e. cylindrical) materials. Such techniques are well described in the technical and patent literature.

Radially expandible unit segment 22 is typically characterized as having a plurality of proximate points 34 and remote points 36. The proximate points 34 are defined herein as those locations on the cut surface of the unit segment 22 axially closest to another longitudinally adjacent unit segment 22. These proximate points 34 are typically those locations most likely to engage the wall of a body lumen during tracking or delivery of the prosthesis. The remote points 36 are defined herein, in the broadest definition, as any point spaced apart from a proximate point 34 on the same element of unit segment 22. Remote points 36 on longitudinally adjacent unit segment 22 are generally locations opposed and furthest from each other. The proximate points 34 and remote points 36 are illustrated in Figs. 2-3B for a variety of segment 22 configurations such as serpentine, zig-zag, and box.

B. *Beams and Expansion Joints*

Referring now to Figs. 1-2, the beams 24 and expansion joints 26 used to couple the unit segments 22 together will now be described. As shown in Fig. 1, the beams 24 are usually straight elongate members in axial alignment with the longitudinal axis of the prosthesis 10. The beams 24 may have a variety of profiles or contours so long as they do not interfere with the function of the prosthesis 10. For example, beams 24 as depicted in Figs. 1 and 4 have narrowed midportions 25 (narrowing is exaggerated for illustrative purposes) to allow the beams to bend around their midpoints. This enhances longitudinal flexibility and prevents interference between the beam 24 and adjacent struts of segment 22 while the prosthesis flexes during delivery or tracking to the luminal target site. The beams 24 are usually axially aligned, connected to the remote points 36 between unit segments 22, and maintain the remote points 36 at a fixed distance at all times including when the prosthesis 10 is radially expanded.

Expansion joints 26, which interconnect proximate points 34 between unit segments 22, are used to prevent fishscaling by maintaining a substantially smooth outer surface on the cylindrical frame 20 when the prosthesis 10 assumes a curved configuration. Fishscaling is prominently exhibited by a prior art prosthesis shown in Fig. 3C where the protruding elements of the prior art prosthesis (available as the Freedom stent from Global Therapeutics Inc. of Broomfield, Colorado) can impede the progress or damage the body lumen if the prosthesis is ever retracted or advanced as indicated by arrow 27. The expansion joints 26 of the present invention minimize any detrimental effects from such protrusions. As shown in Fig. 3D, the expansion joints 26 are designed to connect proximate points 34 to maintain a smooth outer surface for the prosthesis 10, while minimally interfering with the relative axial positioning of the unit segments 22. Preferably, the flexibility of prosthesis 10 allows it to remain in this curved configuration without a tendency to straighten, which will unduly strain a curved body lumen and unnecessarily traumatize the lumen at the ends of the prosthesis.

Referring to Figs. 1-4, the expansion joint 26 may be formed as an "S" shaped member. The "S" configuration allows for axial linear expansion and compression as shown in Figs. 4A-4C. During this linear expansion and compression, as shown in Fig. 3D, the outer surface remains substantially smooth while the expansion joint 26 is expanded or compressed. When the prosthesis 10 assumes a curved configuration, some of the expansion joints 26 are in compression while others are in expansion, maintaining a smooth outer surface on the frame 20 both on the expanded and the compressed sides of the prosthesis. As shown in Figs. 1 and 2, not every proximate point 36 is necessarily connected by an expansion joint 26.

Referring again to Figs. 4A-4C, the expansion joints are generally made weaker than their adjacent struts to facilitate their plastic deformation. In the example shown, the expansion joints are weakened by having reduced widths. The joints 26 may also be weakened by increasing the length of the joint (when fully extended) or by decreasing the thickness of the joint. As shown in Figs. 5-7, the expansion joint 26 may assume a variety of other configurations, such as "U"-shaped, "O"-shaped, or zig-zag shaped joints, with the understanding that the joints maintain a substantially smooth outer surface on the prosthesis 10 during delivery. The expansion joint 26 is preferably adapted for axial compression/expansion and transverse flexing, so as to provide the desired linear and flexural degrees of freedom as noted by arrows 42, 44, and 46. The joints 26 are preferably compliant, malleable structures. Though not restricted in this manner, it is

desired that the beams are the dominant longitudinal structures and are at most, only minimally inhibited by the joints 26.

C. *Pattern*

Aside from the flexural characteristics inherent to the beams and joints, the tracking and expansion characteristics of the prosthesis 10 are typically determined by the positions of the beams 24 and expansion joints 26 between the unit segments 22 (Figs. 1 and 2). For example, a prosthesis 10 using expansion joints 26 will typically have improved tracking capability since the proximal ends are constrained and there is a reduced risk of fishscaling. Likewise, a prosthesis 10 using beams 24 will also have enhanced tracking characteristics by joining adjacent unit segments 22 with a single, long and flexible (malleable) beam providing substantially enhanced articulation between segments during tracking. An important additional advantage of beams 24 relates to improved radial expansion characteristics since prosthesis foreshortening will be substantially compensated by the geometric arrangement of beams and segments.

However, having too many beams 24 and joints 26 or too few joints may create other undesirable qualities such as reduced transverse flexibility characteristics of the prosthesis. Hence, there are performance tradeoffs which must be accounted for in the number of and positioning of beams 24 and joints 26 used in the prosthesis 10.

Referring to Figs. 1 and 2, it should be understood that the beams 24 and expansion joints 26 may be placed in a variety of patterns between the unit segments 22 to balance prosthesis flexibility with competing performance characteristics. In one embodiment shown in Fig. 1, the beams 24 and expansion joints 26 may be linearly aligned in an alternating manner to connect a plurality of adjacent unit segments 22. Adjacent unit segments are connected to one another using only a single beam 24 and one or more expansion joints 26.

Fig. 2 shows a first exemplary embodiment of the prosthesis 10 in a “rolled out” configuration. As shown, adjacent unit segments 22 in Fig. 2 are connected together using both beams 24 and expansion joints 26. As shown in Fig. 2, these beams 24 and expansion joints 26 are not necessarily aligned longitudinally. In this embodiment, only one beam 24 is used per connection between adjacent unit segments 22. This maximizes longitudinal flexibility while providing compensation for longitudinal foreshortening. Further, the beams 24 are in a “laddered” configuration where adjacent beams are laterally (representing the circumferential direction) and longitudinally staggered, with a predetermined amount of longitudinal overlap as shown

in Fig. 2 and in a second exemplary embodiment in Fig. 11. The overlap is preferably at least one-third, more preferably about one-half of the length of the beams 24 when the prosthesis 10 is in a collapsed configuration. Advantageously, positioning beams 24 in a ladder configuration results in a spiralling connecting pattern when the prosthesis is seen in its typical cylindrical configuration. This connecting pattern enhances the transverse flexibility of the prosthesis by distributing the single beams around the circumference of the device.

Axial length compensation for the prosthesis, as it is expanded radially from a collapsed to an expanded or deployed configuration, is conveniently achieved by the previously described interconnecting pattern between beams 24 and unit segments 22. The geometrical relationship is best appreciated in Figs. 8A and 8B which depict three adjacent unit segments 22 both in their collapsed and radially expanded configurations. The axial strut lengths M2 in the expanded configuration are smaller than the axial strut lengths M1 in the collapsed configuration, which is a serious concern in many of the prior art designs. In the present pattern, however, the overall length of the prosthesis, actually grows because the longitudinal distance L2 from the base of a first beam 24a to the base of the next beam 24b is longer than the distance L1 in the collapsed configuration. Furthermore, when the end segments 22 are of the box type as shown in Figs. 1 and 2, there will be a shortening of the longitudinal length of each box section relative to the base of a first beam 24 as shown in Figs. 8C and 8D by the difference in the lengths N1 and N2. The lengthening and shortening of the prosthesis described in relation to Figs. 8A/8B and Figs. 8C/8D, respectively, can be used advantageously in attaining optimal length compensation when the prosthesis is expanded or deployed.

III. Axially Selective Radial Stiffness

Referring now to Figs. 9 and 10, a prostheses having axially selective radial stiffnesses can be adapted to control geometrical characteristics resulting in undesired tracking performance. One factor in determining radial stiffness is the type of material used to fabricate the prosthesis. The material is preferably a material such as 316L stainless steel which in its annealed condition is strong yet malleable and will therefore remain in an expanded configuration with a minimum of recoil. Of course, the stronger the material, the harder the prosthesis will be to expand. Another factor in radial stiffness is the length of the struts 102 used in the unit segments 22. The shorter the struts 102, the less leverage or mechanical advantage it will have to deform the hinge element.

Therefore shorter struts will require greater forces than longer struts to expand the hinge element between two struts. A further factor involves the design of the hinges 104 connecting adjacent struts 102. The longer, narrower, and thinner the hinge 104 is, as indicated by arrows 106, 107, and 108 respectively, the weaker the hinge will be. The shorter, wider, and thicker the hinge 104 is, the stiffer the hinge 104 will be.

Referring to Figs. 10A and 10B, a prosthesis 10 having axially selective radial expansion stiffnesses will be described. As shown in Fig. 10A, conventional luminal prostheses have a tendency to flare near the distal end 110 and proximal end 112, especially during tracking through tortuous anatomy, but also when radially expanded by a balloon. This produces an hourglass or double trumpet configuration which may cause trauma to the body lumen wall and even inhibit the progress of the catheter mounted prosthesis during tracking of the prosthesis to the target site. It may also cause excessive end deformation when being expanded, thus potentially being the focus of a stronger restenotic effect. Flaring or trumpeting occurs because the prosthesis resists excessive bending while tracking through tortuous pathways and the struts on the ends of the prosthesis will preferably deform (as illustrated in Fig. 10A), causing the prosthesis to assume a double trumpet shape rather than remaining in the desired cylindrical configuration along its entire length. This occurs particularly in the prior art because the unit segments in the middle of the prosthesis 10 are connected to or constrained by adjacent unit segments and provide transverse rigidity to the prosthesis while those segments on the ends are cantilevered, with only one side constrained. Hence they are more susceptible to deformation during tracking. Because these prostheses are typically made from malleable materials, they remain deformed even though the delivery catheter may have returned to a straight configuration.

In a preferred embodiment of the prosthesis 10, unit segments near the vicinity of the distal end 111 and proximal end 113 have a higher radial stiffness than the unit segments near the center or in the midsection 27 of the prosthesis 10. Although the prosthesis is not limited in this manner, the additional radial stiffness minimizes the observed flaring. Radial stiffness may be increased in a variety of ways, such as using longitudinally shorter unit segments or by altering the geometry, i.e. widths, lengths, and thicknesses, of the outermost components of the unit segments. The amount of force required to expand the prosthesis may therefore vary over the length of the prosthesis.

In one embodiment as shown in Fig. 10B, end rings 120 and 121 which form the distal end and the proximal end of the prosthesis 10 incorporate a plurality of

substantially longitudinal portions or struts 122 which are shorter in length than the longitudinal portions 130 characteristic of the unit segments 22 near the middle of the prosthesis. Although the portions 122 may assume a variety of lengths, the portions are typically half as long as those portions 130 in unit segments 22. These end rings 120 and 121 with the shorter and therefore stronger longitudinal portions will preferably become only minimally flared during the tracking and the expansion of the prosthesis. The end rings 120 and 121 having higher radial stiffness are preferably included in embodiments of the prosthesis 10, as shown in Figs. 1 and 2. The end rings 120 and 121 may have a serpentine, zig-zag, or other similar configuration.

In the embodiment of Fig. 11, it is shown that rings 120 and 121 having shorter struts 122 may be coupled to adjacent unit segments by a combination of a single beam 24 and expansion joints 26. One ring 120 or 121 may be directly connected to a unit segment 22, thus forming an articulated structure with the unit segment. Rings 120 or 121 may also be coupled to unit segment 22 by expansion joints 26 to prevent fishscaling without inhibiting transverse flexibility.

In an alternative embodiment, the serpentine ring may incorporate other elements to increase radial stiffness. For example, in Fig. 13, the distal end and proximal end of the prosthesis 10 may be covered by annular sheaths 130 and 131 made of expansible material that radially constrains the ends to minimize flaring and will typically become implanted in body lumen together with the prosthesis. Other suitable devices and methods for constraining the expansion of unit segments 120, 121, and 22, such as expansion limiting hinges, may be found in commonly assigned, co-pending U.S. Patent application Serial No. 08/691,661, filed August 2, 1996 (Attorney Docket No. 15509-003900), the complete disclosure of which was previously incorporated herein.

IV. Endolumenal Delivery and Expansion

As shown in Fig. 13, in a preferred embodiment, the prosthesis 10 is preferably crimped onto a collapsed expansible inflation member 80 having a typically cylindrical inflation section 82 which is typically located at the distal end of a catheter 100 (Fig. 14). It should be understood, however, that the prosthesis 10 may be coupled to inflation member 80 by other methods known in the art, such as stent delivery sleeves as described in commonly assigned U.S. Patent No. 5,599,306 or commonly assigned, copending U.S. Patent Application Serial No. 08/704,801, filed August 26, 1996 (Attorney Docket No. 15509-002810), the complete disclosures of which are incorporated

herein by reference. In a preferred embodiment, the prosthesis 10 as mounted over an expandable inflation member 80, such as a non-compliant elastomeric balloon, is designed to track through curved and tortuous body lumens as shown in Fig. 14 to reach a target site T. As shown, the expansion joints 26 prevent the prosthesis 10 from engaging the lumen wall when the prosthesis 10 is in a curved configuration. Additionally, the prosthesis 10 preferably includes stiffened radial ends to reduce prosthesis trumpeting. These features improve tracking of the prosthesis 10 through the lumen. When the prosthesis and balloon reach the desired target site T, the expandable member 80 will be expanded to deploy the prosthesis 10 as shown in Figs. 15A-15D. After the prosthesis 10 has been deployed, the balloon or expandable member 80 will be deflated and removed along with the catheter from the body lumen. The prosthesis 10 will remain in the body lumen to maintain the lumen patency.

In preferred embodiments of the present invention, the prosthesis 10 is mounted on a inflation member 80 of “matching” length to minimize dissectogenic balloon expansion that is characteristic of known catheter/stent assemblies. “Matching” is defined as having an expandable member 80 with an inflation section 82 (cylindrical, tapered, or other shape) of substantially the same length as the length of the prosthesis 10. As can be observed in Figs. 16A-16C, even when the end sections of the prosthesis are strengthened, the diameter of the outer ends of a conventional balloon 86 exceeds the outer diameter of the prosthesis as the balloon attempts to expand the prosthesis and even following full expansion. The balloon’s excessive radial expansion results from inflating portions of the balloon unconstrained by the prosthesis. High pressure inflation (in the range of 10-20 atmospheres) to fully expand the prosthesis into the body lumen may cause these unconstrained portions or bulbs 84 to reach a size sufficient to damage or dissect the body lumen, particularly at the distal end. To eliminate these bulbs 84, a system 200, shown in Figs. 15A-15D and 17A-17C, according to the present invention preferably uses an expandable inflation member 80 having a cylindrical or other shaped inflation section 82 with approximately the same longitudinal length as that of the prosthesis 10. The “inflation section” may be defined as those areas of the inflation member 80 which can extend beyond the outer diameter of the prosthesis 10 under typical high pressure inflation if unconstrained. Although not limited in this manner, the distal and proximal ends or tips of the member 80 are typically molded and will not expand beyond the diameter of the member. The cylindrical inflation section 82 is no more than about 1.0 mm longer than the prosthesis on each end, preferably no more than about 0.5

mm longer, and most preferably the same length as the prosthesis. As shown in Figs. 17A-17C, matching the length of the expanding balloon portion with the length of the prosthesis significantly reduces undesired balloon configurations 84 as the prosthesis 10 is fully expanded in place. It should be understood that the inflation section 82 may assume a variety of configurations once expanded.

In a preferred embodiment, a system 200 with a prosthesis 10 and expandible member 80 of similar lengths comes with the prosthesis 10 coupled to the expandible member 80. Alternatively, the prosthesis 10 may come as a separate entity that is subsequently mounted onto a suitable expandible inflation member 80. Referring to Figs. 18A-18C, a method for mounting a prosthesis 10 onto a suitable inflation member 80 includes selecting an expandible inflation member having an inflation section 82 of about the same longitudinal length as the length of a prosthesis 10 (as discussed above). The expandible inflation member 80 is positioned in a longitudinal lumen of said prosthesis 10 prior to the clinical intervention. The position of the longitudinal length of the prosthesis 10 is aligned with the length of the inflation section 82 of the inflation member 80. The prosthesis 10 is then mounted onto the inflation member 80 either by hand crimping or preferably with a crimping tool (not shown). As shown, the inflation member 80 preferably comes with a catheter 100. It is understood, however, that the prosthesis may be premounted at the factory on a delivery device such as a balloon or a sleeve catheter.

Referring to Fig. 19, a prosthesis 10 according to the present invention may be packaged together with instructions for use (IFU) in a kit as shown in Fig. 12. A conventional package, which may be a pouch 202 or any other suitable package, such as a tray, box, tube, or the like, may be used to contain the prosthesis 10 and IFU 204, where the IFU may be printed on a separate sheet and/or may be printed on the packaging itself. The kit may also include a mounting tool 206 such as a crimping device and/or an expandible inflation member 80 which may be permanently or releasably coupled to the prosthesis 10. Typically, the expandible member 80 is attached to catheter 100. The instructions will set forth any of the aspects of the method of the present invention described above, including the method for mounting a prosthesis 10.

Further embodiments of the prosthesis 10 of the present invention may have expanded configurations designed to address specific interventional needs. For example, expanded prostheses configurations may be designed to match the shape of the lumens for which they are targeted. Many body lumens have irregular configurations,

and it has been suggested that over 40% of all blood vessels in the body are tapered. To match these body lumen shapes, a prosthesis according to the present invention are preferably be mounted on an expandable balloon 90 which will shape the expanded configuration of the prosthesis as shown in Figs. 20A-20D respectively. These balloons 90 such as the Banka tapered balloon from C.R. Bard, Inc. of Billerica, Massachusetts or the CAT balloon from CardioVascular Dynamics, Inc. of Irvine, California may expand into tapered or other desired configurations. A prosthesis of the present invention mounted on such a balloon 90 will have a matching expanded configuration.

Advantageously, matching the prosthesis 10 to the body lumen reduces stress concentrations which may occur when the body lumen is excessively distended by nonconforming (typically cylindrically) expanded prosthesis. A shaped prosthesis further allows for effective scaffolding of lesions having tapered configurations, grant more effective support of lesions at anastomosis sites, and more accurate sizing and scaffolding of ostial lesions. In contrast to conventionally delivered prosthesis, a prosthesis shaped through specific delivery means can concentrate the majority of the supporting force more directly at a lesion site, sparing the surrounding luminal wall from potentially damaging dilation forces. It should be understood that an unlimited number of results and configurations can be created by varying the radial stiffnesses along the length of the prosthesis and the shape of the delivery system.

Additionally, as can be seen in Figs. 20A-20F, the strut lengths can be varied to optimize the dilatation and support forces of the shaped prosthesis. Varying the strut lengths can create a radial stiffness gradient between the unit segments to further enhance luminal scaffolding. The various prostheses may have struts 212 and 214 with shorter and longer lengths in a tapered expanded configuration (Fig. 20A). Other tapered expanded configurations may have short struts S with long struts L (Fig. 20B), all long struts L (Fig. 20C), or short struts with gradually longer struts L/L+/L++ (Fig. 20D). In cylindrical configurations, the prosthesis 10 may have short struts S and long struts L (Fig. 20E) or short struts S, long struts L, and medium struts M (Fig. 20F). As shown, any combination of strut lengths may be used to optimize desired prosthesis characteristics.

V. Radiopaque Marking Schemes

Proper positioning of a prosthesis in a body lumen can be critical to attain the optimal therapeutic effect from the device. For example, it is sometimes necessary to

juxtapose several prostheses in the same body lumen to treat a long lesion. This may require abutting the end of one prosthesis against the end of another prosthesis or slightly overlapping their ends. To visualize the position of these prostheses as they are delivered into the body lumen, physicians use fluoroscopy or angiography to illuminate the devices in the body lumen. The prostheses preferably have some radiopaque marking features or may be made from radiopaque materials to be detectable by a fluoroscope or similar visualization devices.

Referring to Figs. 22A-22E, a method for plating a typical prosthesis made from stainless steel with radiopaque material, such as gold, platinum, platinum/iridium, tungsten, tantalum, or the like, will now be described. The method of the present invention creates a prosthesis with a coating of radiopaque material having an axially selective thickness. It should be understood, however, that the method is not limited to thickness variations in the axial direction and may be used to create an unlimited number of thickness configurations. Preferably, the prosthesis is entirely covered with a layer of radiopaque material while having thicker deposits of the same or other materials near its ends and having thinner deposits over the remainder, typically midsection, of the device. When the coating material is gold, the thickness near the ends 111 and 113 is preferably between 0.0003 and 0.0009 inches, more preferably between 0.0004 and 0.0007 inches. Thicknesses over the remainder of the prosthesis may be in the range of 0.0002 to 0.0004 inches. The thicker deposits near the ends of the prosthesis make the ends more radiopaque and thus create a stronger image, facilitating the positioning of the prosthesis in its desired location. The middle area 304 is also preferably coated so as to be more radiopaque than the uncoated material under the fluoroscope, but permitting sufficient radiolucency so that the lumen inside the prosthesis may still be inspected fluoroscopically. Alternatively, the middle area 304 may be left uncoated while only the ends of the prosthesis remain coated to achieve an optimal axial radiopacity distribution. Visualization through this middle area 304 may be crucial for observing future restenosis or hyperplasia within the prosthesis. Coating the entire prosthesis at a uniform thickness using the optimal thickness applied to the ends would likely obscure such visualization. Having an axially selective coating customizes the prosthesis to the desired task. It should be understood that the present method may be used to add materials of a variety of thicknesses to a prosthesis.

One embodiment of the present method uses electroplating steps to add radiopaque material to the prosthesis. It should be understood, however, that other

processes known in the art may also be adapted according to the present invention. The method comprises immersing the completed prosthesis (i.e. cut and polished) in an electrolyte and electroplating the entire prosthesis with a layer 300 of radiopaque material such as gold at a preferred thickness of 0.0003 inches (Fig. 21A). The prosthesis is shown in cross-section, and the plating is shown disproportionately thick for better clarity. The portions of the prosthesis 10 desired to have greater thickness (in this example the two ends) are then covered with a resist material 302 to protect the covered materials from plating removal or plating addition (Fig. 21B). Such resist material 302 may be for example Microposit® FSC® Surface Coating manufactured by the Shipley Company in Marlborough, Massachusetts. The electroplating process is then reversed to remove radiopaque material not covered with the resist material. In this example of Fig. 21C, it is shown completely removed. The resist material is then removed, leaving behind a prosthesis 10 with select areas covered with a layer 300 of radiopaque material while other areas 304 remain bare (Fig. 21D). The entire prosthesis 10 is then covered with another layer 306 of radiopaque material, such as gold at 0.0003 inches thickness (Fig. 21E). The resulting embodiment of the prosthesis will thus have ends coated with 0.0006 inches of gold, while the remainder of the prosthesis is covered with 0.0003 inches of gold. If a radiopaque coating is desired only at the ends of the prosthesis, the initial coating as shown in Fig. 21A may be made thicker, such as 0.0006 inches of gold, and the final coating step in Fig. 21E may be omitted. This will result in a prosthesis having a coating of 0.0006 inches of gold at its ends, and not coating the middle area.

Alternatively, another method for creating selective coatings of radiopaque material may use a combination of electrolytic deposition, electroless dipping, and sputter processes (Figs. 22A-22C). For example, both ends of the prosthesis are sequentially dipped in radiopaque material, resulting in a prosthesis with a bare middle area 310 and two covered ends 312. This prosthesis can then be entirely recoated using a sputtering process in a vacuum chamber 314 (Fig. 22B). This results in a prosthesis entirely covered with radiopaque material, but having thicker, more opaque ends (Fig. 22C). Although the process using electroplating and the resist material is more flexible as to the shape and location of the areas with thicker coatings, the dipping and/or sputtering processes may also be used to create a prosthesis entirely covered with radiopaque material but having thicker coatings on the ends. It should be understood these method steps may be performed in a variety of different sequences, such as coating the entire prosthesis first and then coating the ends, to create the desired radiopaque coating distribution. Similar

thicknesses to gold may be used with other commonly used radiopaque materials such as platinum or platinum/iridium alloys.

Although the foregoing invention has been described in some detail by way of illustration and example, for purposes of clarity of understanding, it will be obvious that certain changes and modifications may be practiced within the scope of the appended claims. For example, the prostheses may be sized as appropriate for use in a variety of body lumens such as the aorta or other vasculature in the body.

1
2
3
4
5
6
7
8
9
10
11
12
13
14
15
16
17
18
19
20
21
22
23
24
25
26
27
28
29
30
31
32
33
34
35
36
37
38
39
40
41
42
43
44
45
46
47
48
49
50
51
52
53
54
55
56
57
58
59
60
61
62
63
64
65
66
67
68
69
70
71
72
73
74
75
76
77
78
79
80
81
82
83
84
85
86
87
88
89
90
91
92
93
94
95
96
97
98
99
100
101
102
103
104
105
106
107
108
109
110
111
112
113
114
115
116
117
118
119
120
121
122
123
124
125
126
127
128
129
130
131
132
133
134
135
136
137
138
139
140
141
142
143
144
145
146
147
148
149
150
151
152
153
154
155
156
157
158
159
160
161
162
163
164
165
166
167
168
169
170
171
172
173
174
175
176
177
178
179
180
181
182
183
184
185
186
187
188
189
190
191
192
193
194
195
196
197
198
199
200
201
202
203
204
205
206
207
208
209
210
211
212
213
214
215
216
217
218
219
220
221
222
223
224
225
226
227
228
229
230
231
232
233
234
235
236
237
238
239
240
241
242
243
244
245
246
247
248
249
250
251
252
253
254
255
256
257
258
259
260
261
262
263
264
265
266
267
268
269
270
271
272
273
274
275
276
277
278
279
280
281
282
283
284
285
286
287
288
289
290
291
292
293
294
295
296
297
298
299
300
301
302
303
304
305
306
307
308
309
310
311
312
313
314
315
316
317
318
319
320
321
322
323
324
325
326
327
328
329
330
331
332
333
334
335
336
337
338
339
340
341
342
343
344
345
346
347
348
349
350
351
352
353
354
355
356
357
358
359
360
361
362
363
364
365
366
367
368
369
370
371
372
373
374
375
376
377
378
379
380
381
382
383
384
385
386
387
388
389
390
391
392
393
394
395
396
397
398
399
400
401
402
403
404
405
406
407
408
409
410
411
412
413
414
415
416
417
418
419
420
421
422
423
424
425
426
427
428
429
430
431
432
433
434
435
436
437
438
439
440
441
442
443
444
445
446
447
448
449
450
451
452
453
454
455
456
457
458
459
460
461
462
463
464
465
466
467
468
469
470
471
472
473
474
475
476
477
478
479
480
481
482
483
484
485
486
487
488
489
490
491
492
493
494
495
496
497
498
499
500
501
502
503
504
505
506
507
508
509
510
511
512
513
514
515
516
517
518
519
520
521
522
523
524
525
526
527
528
529
530
531
532
533
534
535
536
537
538
539
540
541
542
543
544
545
546
547
548
549
550
551
552
553
554
555
556
557
558
559
560
561
562
563
564
565
566
567
568
569
570
571
572
573
574
575
576
577
578
579
580
581
582
583
584
585
586
587
588
589
590
591
592
593
594
595
596
597
598
599
600
601
602
603
604
605
606
607
608
609
610
611
612
613
614
615
616
617
618
619
620
621
622
623
624
625
626
627
628
629
630
631
632
633
634
635
636
637
638
639
640
641
642
643
644
645
646
647
648
649
650
651
652
653
654
655
656
657
658
659
660
661
662
663
664
665
666
667
668
669
670
671
672
673
674
675
676
677
678
679
680
681
682
683
684
685
686
687
688
689
690
691
692
693
694
695
696
697
698
699
700
701
702
703
704
705
706
707
708
709
710
711
712
713
714
715
716
717
718
719
720
721
722
723
724
725
726
727
728
729
730
731
732
733
734
735
736
737
738
739
740
741
742
743
744
745
746
747
748
749
750
751
752
753
754
755
756
757
758
759
760
761
762
763
764
765
766
767
768
769
770
771
772
773
774
775
776
777
778
779
780
781
782
783
784
785
786
787
788
789
790
791
792
793
794
795
796
797
798
799
800
801
802
803
804
805
806
807
808
809
810
811
812
813
814
815
816
817
818
819
820
821
822
823
824
825
826
827
828
829
830
831
832
833
834
835
836
837
838
839
840
841
842
843
844
845
846
847
848
849
850
851
852
853
854
855
856
857
858
859
860
861
862
863
864
865
866
867
868
869
870
871
872
873
874
875
876
877
878
879
880
881
882
883
884
885
886
887
888
889
890
891
892
893
894
895
896
897
898
899
900
901
902
903
904
905
906
907
908
909
910
911
912
913
914
915
916
917
918
919
920
921
922
923
924
925
926
927
928
929
930
931
932
933
934
935
936
937
938
939
940
941
942
943
944
945
946
947
948
949
950
951
952
953
954
955
956
957
958
959
960
961
962
963
964
965
966
967
968
969
970
971
972
973
974
975
976
977
978
979
980
981
982
983
984
985
986
987
988
989
990
991
992
993
994
995
996
997
998
999
1000
1001
1002
1003
1004
1005
1006
1007
1008
1009
1010
1011
1012
1013
1014
1015
1016
1017
1018
1019
1020
1021
1022
1023
1024
1025
1026
1027
1028
1029
1030
1031
1032
1033
1034
1035
1036
1037
1038
1039
1040
1041
1042
1043
1044
1045
1046
1047
1048
1049
1050
1051
1052
1053
1054
1055
1056
1057
1058
1059
1060
1061
1062
1063
1064
1065
1066
1067
1068
1069
1070
1071
1072
1073
1074
1075
1076
1077
1078
1079
1080
1081
1082
1083
1084
1085
1086
1087
1088
1089
1090
1091
1092
1093
1094
1095
1096
1097
1098
1099
1100
1101
1102
1103
1104
1105
1106
1107
1108
1109
1110
1111
1112
1113
1114
1115
1116
1117
1118
1119
1120
1121
1122
1123
1124
1125
1126
1127
1128
1129
1130
1131
1132
1133
1134
1135
1136
1137
1138
1139
1140
1141
1142
1143
1144
1145
1146
1147
1148
1149
1150
1151
1152
1153
1154
1155
1156
1157
1158
1159
1160
1161
1162
1163
1164
1165
1166
1167
1168
1169
1170
1171
1172
1173
1174
1175
1176
1177
1178
1179
1180
1181
1182
1183
1184
1185
1186
1187
1188
1189
1190
1191
1192
1193
1194
1195
1196
1197
1198
1199
1200
1201
1202
1203
1204
1205
1206
1207
1208
1209
1210
1211
1212
1213
1214
1215
1216
1217
1218
1219
1220
1221
1222
1223
1224
1225
1226
1227
1228
1229
1230
1231
1232
1233
1234
1235
1236
1237
1238
1239
1240
1241
1242
1243
1244
1245
1246
1247
1248
1249
1250
1251
1252
1253
1254
1255
1256
1257
1258
1259
1260
1261
1262
1263
1264
1265
1266
1267
1268
1269
1270
1271
1272
1273
1274
1275
1276
1277
1278
1279
1280
1281
1282
1283
1284
1285
1286
1287
1288
1289
1290
1291
1292
1293
1294
1295
1296
1297
1298
1299
1300
1301
1302
1303
1304
1305
1306
1307
1308
1309
1310
1311
1312
1313
1314
1315
1316
1317
1318
1319
1320
1321
1322
1323
1324
1325
1326
1327
1328
1329
1330
1331
1332
1333
1334
1335
1336
1337
1338
1339
1340
1341
1342
1343
1344
1345
1346
1347
1348
1349
1350
1351
1352
1353
1354
1355
1356
1357
1358
1359
1360
1361
1362
1363
1364
1365
1366
1367
1368
1369
1370
1371
1372
1373
1374
1375
1376
1377
1378
1379
1380
1381
1382
1383
1384
1385
1386
1387
1388
1389
1390
1391
1392
1393
1394
1395
1396
1397
1398
1399
1400
1401
1402
1403
1404
1405
1406
1407
1408
1409
1410
1411
1412
1413
1414
1415
1416
1417
1418
1419
1420
1421
1422
1423
1424
1425
1426
1427
1428
1429
1430
1431
1432
1433
1434
1435
1436
1437
1438
1439
1440
1441
1442
1443
1444
1445
1446
1447
1448
1449
1450
1451
1452
1453
1454
1455
1456
1457
1458
1459
1460
1461
1462
1463
1464
1465
1466
1467
1468
1469
1470
1471
1472
1473
1474
1475
1476
1477
1478
1479
1480
1481
1482
1483
1484
1485
1486
1487
1488
1489
1490
1491
1492
1493
1494
1495
1496
1497
1498
1499
1500
1501
1502
1503
1504
1505
1506
1507
1508
1509
1510
1511
1512
1513
1514
1515
1516
1517
1518
1519
1520
1521
1522
1523
1524
1525
1526
1527
1528
1529
1530
1531
1532
1533
1534
1535
1536
1537
1538
1539
1540
1541
1542
1543
1544
1545
1546
1547
1548
1549
1550
1551
1552
1553
1554
1555
1556
1557
1558
1559
1560
1561
1562
1563
1564
1565
1566
1567
1568
1569
1570
1571
1572
1573
1574
1575
1576
1577
1578
1579
1580
1581
1582
1583
1584
1585
1586
1587
1588
1589
1590
1591
1592
1593
1594
1595
1596
1597
1598
1599
1600
1601
1602
1603
1604
1605
1606
1607
1608
1609
1610
1611
1612
1613
1614
1615
1616
1617
1618
1619
1620
1621
1622
1623
1624
1625
1626
1627
1628
1629
1630
1631
1632
1633
1634
1635
1636
1637
1638
1639
1640
1641
1642
1643
1644
1645
1646
1647
1648
1649
1650
1651
1652
1653
1654
1655
1656
1657
1658
1659
1660
1661
1662
1663
1664
1665
1666
1667
1668
1669
1670
1671
1672
1673
1674
1675
1676
1677
1678
1679
1680
1681
1682
1683
1684
1685
1686
1687
1688
1689
1690
1691
1692
1693
1694
1695
1696
1697
1698
1699
1700
1701
1702
1703
1704
1705
1706
1707
1708
1709
1710
1711
1712
1713
1714
1715
1716
1717
1718
1719
1720
1721
1722
1723
1724
1725
1726
1727
1728
1729
1730
1731
1732
1733
1734
1735
1736
1737
1738
1739
1740
1741
1742
1743
1744
1745
1746
1747
1748
1749
1750
1751
1752
1753
1754
1755
1756
1757
1758
1759
1760
1761
1762
1763
1764
1765
1766
1767
1768
1769
1770
1771
1772
1773
1774
1775
1776
1777
1778
1779
1780
1781
1782
1783
1784
1785
1786
1787
1788
1789
1790
1791
1792
1793
1794
1795
1796
1797
1798
1799
1800
1801
1802
1803
1804
1805
1806
1807
1808
1809
1810
1811
1812
1813
1814
1815
1816
1817
1818
1819
1820
1821
1822
1823
1824
1825
1826
1827
1828
1829
1830
1831
1832
1833
1834
1835
1836
1837
1838
1839
1840
1841
1842
1843
1844
1845
1846
1847
1848
1849
1850
1851
1852
1853
1854
1855
1856
1857
1858
1859
1860
1861
1862
1863
1864
1865
1866
1867
1868
1869
1870
1871
1872
1873
1874
1875
1876
1877
1878
1879
1880
1881
1882
1883
1884
1885
1886
1887
1888
1889
1890
1891
1892
1893
1894
1895
1896
1897
1898
1899
1900
1901
1902
1903
1904
1905
1906
1907
1908
1909
1910
1911
1912
1913
1914
1915
1916
1917
1918
1919
1920
1921
1922
1923
1924
1925
1926
1927
1928
1929
1930
1931
1932
1933
1934
1935
1936
1937
1938
1939
1940
1941
1942
1943
1944
1945
1946
1947
1948
1949
1950
1951
1952
1953
1954
1955
1956
1957
1958
1959
1960
1961
1962
1963
1964
1965
1966
1967
1968
1969
1970
1971
1972
1973
1974
1975
1976
1977
1978
1979
1980
1981
1982
1983
1984
1985
1986
1987
1988
1989
1990
1991
1992
1993
1994
1995
1996
1997
1998
1999
2000
2001
2002
2003
2004
2005
2006
2007
2008
2009
2010
2011
2012
2013
2014
2015
2016
2017
2018
2019
2020
2021
2022
2023
2024
2025
2026
2027
2028
2029
2030
2031
2032
2033
2034
2035
2036
2037
2038
2039
2040
2041
2042
2043
2044
2045
2046
2047
2048
2049
2050
2051
2052
2053
2054
2055
2056
2057
2058
2059
2060
2061
2062
2063
2064
2065
2066
2067
2068
2069
2070
2071
2072
2073
2074
2075
2076
2077
2078
2079
2080
2081
2082
2083
2084
2085
2086
2087
2088
2089
2090
2091
2092
2093
2094
2095
2096
2097
2098
2099
2100
2101
2102
2103
2104
2105
2106
2107
2108
2109
2110
2111
2112
2113
2114
2115
2116
2117
2118
2119
2120
2121
2122
2123
2124
2125
2126
2127
2128
2129
2130
2131
2132
2133
2134
2135
2136
2137
2138
2139
2140
2141
2142
2143
2144
2145
2146
2147
2148
2149
2150
2151
2152
2153
2154
2155
2156
2157
2158
2159
2160
2161
2162
2163
2164
2165
2166
2167
2168
2169
2170
2171
2172
2173
2174
2175
2176
2177
2178
2179
2180
2181
2182
2183
2184
2185
2186
2187
2188
2189
2190
2191
2192
2193
2194
2195
2196
2197
2198
2199
2200
2201
2202
2203
2204
2205
2206
2207
2208
2209
2210
2211
2212
2213
2214
2215
2216
221

WHAT IS CLAIMED IS:

1 1. A radially expansible luminal prosthesis comprising:
2 a cylindrical frame having a distal end, a proximal end, and an outer
3 surface for insertion into a body lumen, wherein said frame comprises a radiopaque
4 material which varies in thickness over an axial length of the cylindrical frame so that the
5 radiopacity of the frame varies correspondingly.

1 2. A radially expansible luminal prosthesis as in claim 1, wherein the
2 cylindrical frame comprises stainless steel and a radiopaque material is coated over the
3 stainless steel.

1 3. A radially expansible luminal prosthesis as in claim 2, wherein the
2 radiopaque material is selected from the group consisting of gold, platinum,
3 platinum/iridium, tungsten, and tantalum.

1 4. A radially expansible luminal prosthesis as in any of claims 1 to 3,
2 wherein the radiopaque material is thicker near the ends of the cylindrical frame than over
3 the midsection.

1 5. An improved radially expansible luminal prosthesis of the type
2 comprising a cylindrical frame having a distal end, a proximal end, and a midsection
3 therebetween, wherein the cylindrical frame is modified to be radiopaque at each end but
4 to remain sufficiently radiolucent over the midsection to permit fluoroscopic viewing of a
5 blood vessel lumen in which the prosthesis is implanted.

RADIALLY EXPANSIBLE VESSEL SCAFFOLD HAVING MODIFIED RADIOCAPACITY

ABSTRACT OF THE DISCLOSURE

The present invention provides improved prostheses and methods for their endolumenal placement within body lumens, particularly blood vessels. In one embodiment, the prosthesis of the present invention comprises a plurality of radially expansible rings having, a plurality of beams connecting axially remote points on adjacent rings, and a plurality of expansion joints connecting axially proximate points on adjacent rings. The beams maintain the remote points at a fixed distance when the prosthesis is radially expanded and the expansion joints allow for relative movement of the proximate points during delivery of the prosthesis. The combination of the beams and expansion joints minimizes the risk of injury to the body lumen during delivery of the prosthesis to a target site and provides improved tracking capabilities.

PA 3091205 v1




FIG. 1

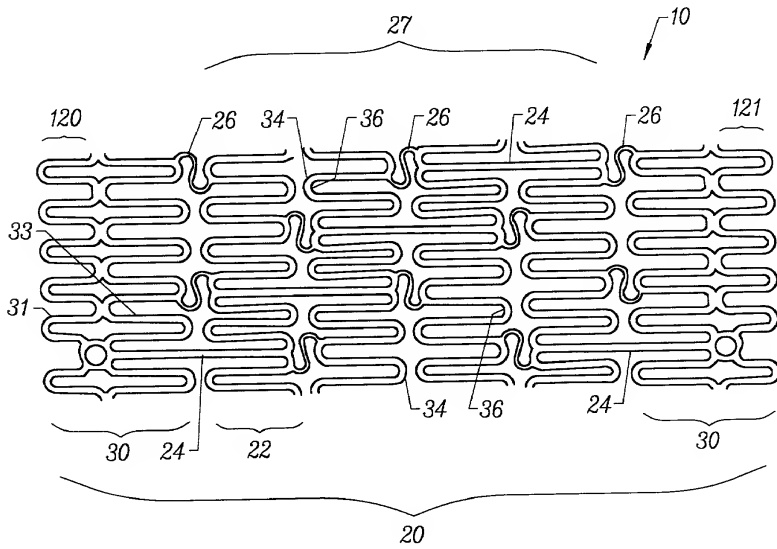


FIG. 2




FIG. 3A




FIG. 3B

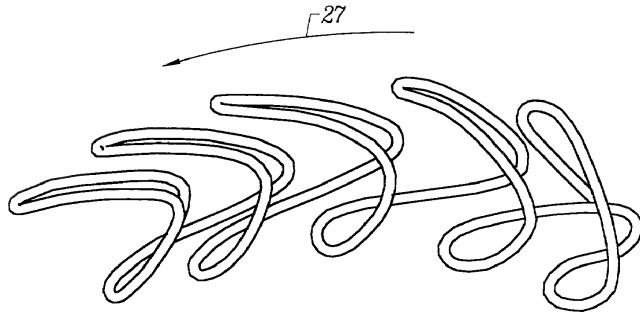


FIG. 3C
PRIOR ART

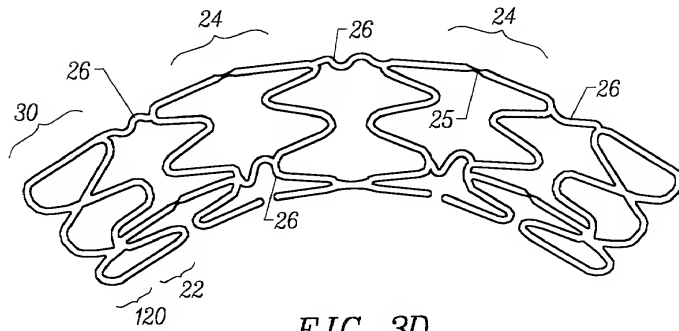


FIG. 3D

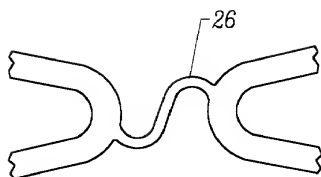


FIG. 4A

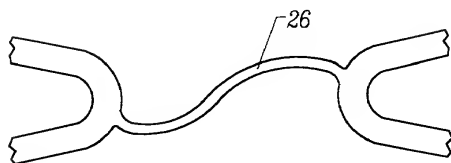


FIG. 4B




FIG. 4C

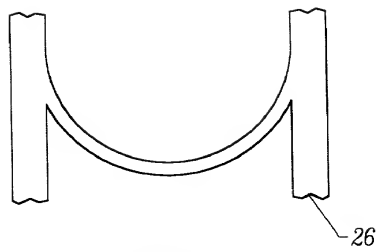


FIG. 5

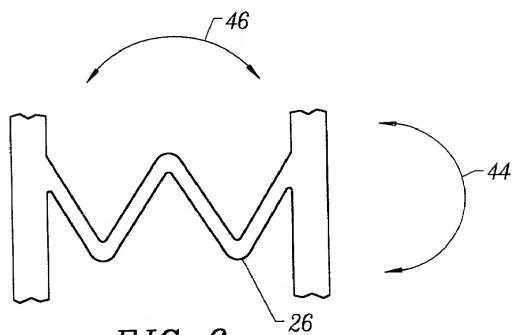


FIG. 6

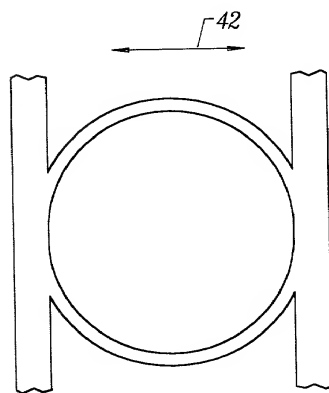


FIG. 7

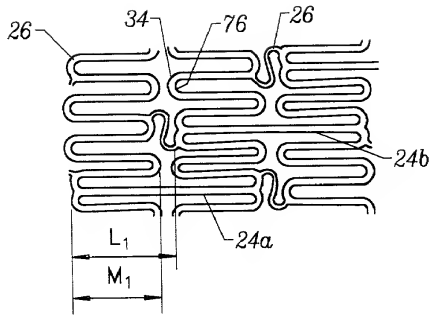


FIG. 8A

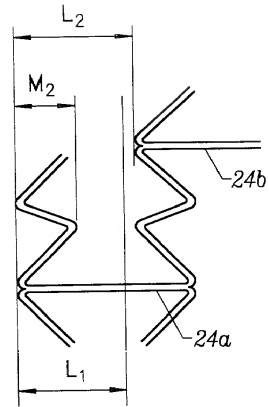


FIG. 8B




FIG. 8C




FIG. 8D

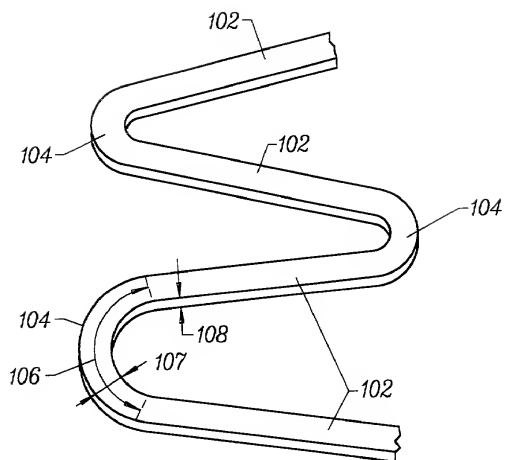


FIG. 9

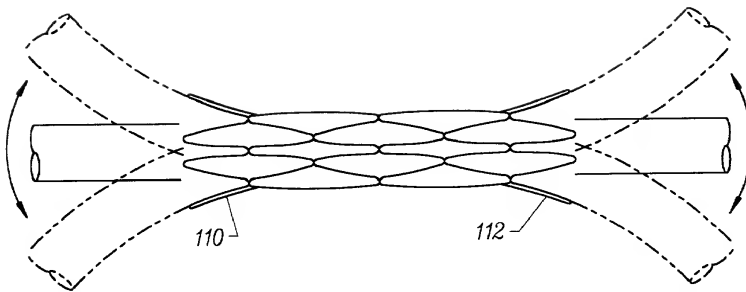


FIG. 10A
PRIOR ART

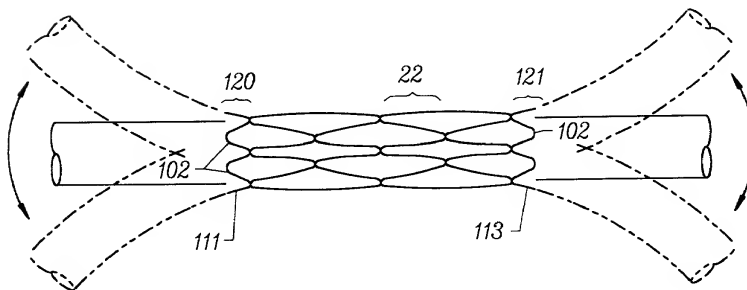


FIG. 10B

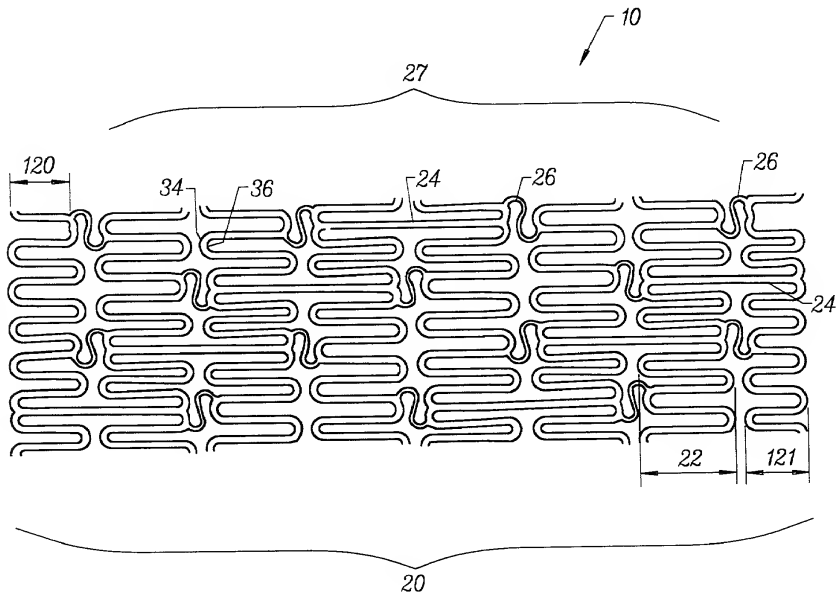


FIG. 11

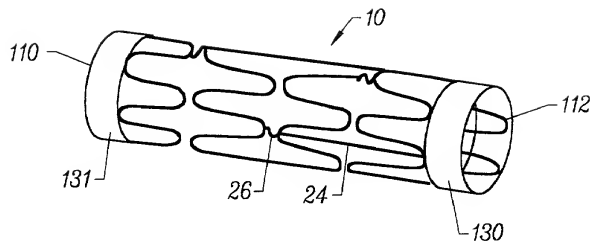


FIG. 12

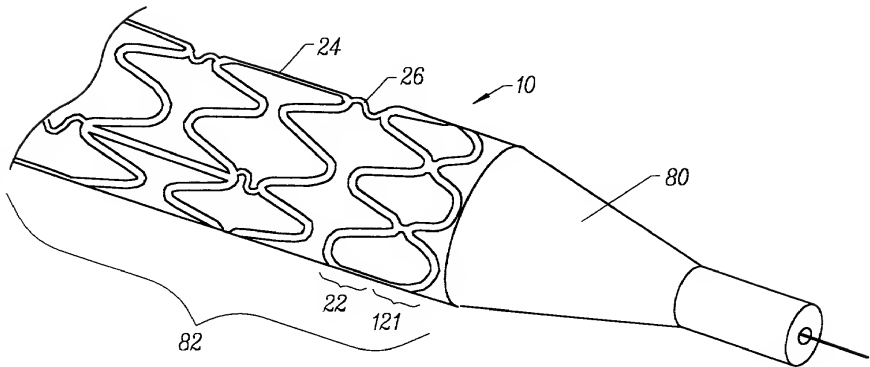


FIG. 13

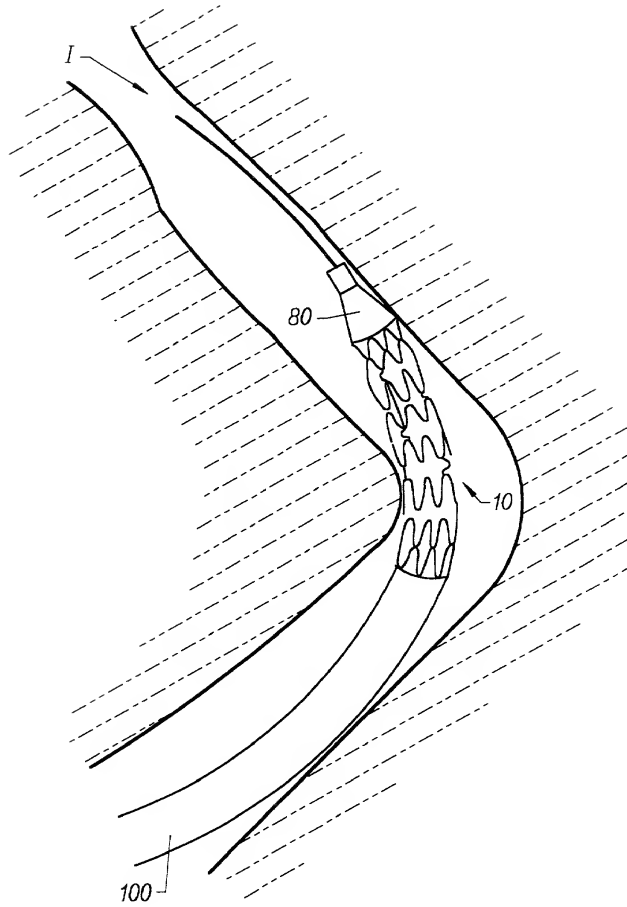


FIG. 14

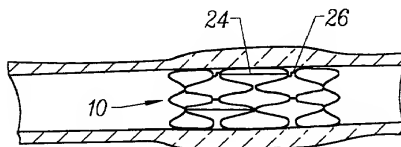
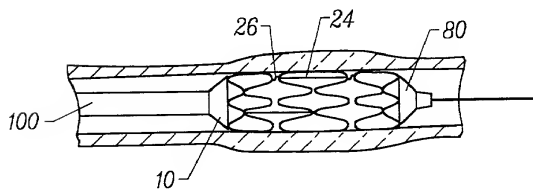
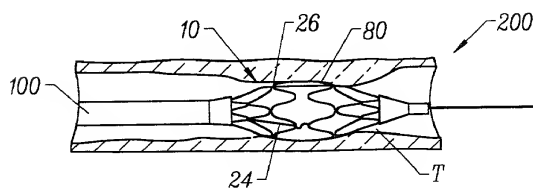
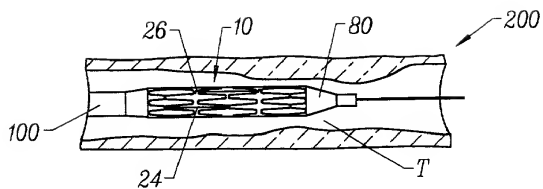




FIG. 16A

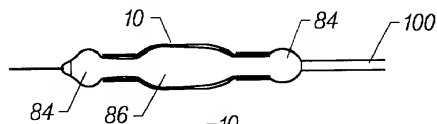


FIG. 16B

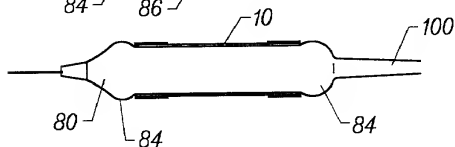


FIG. 16C

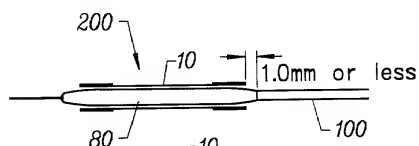


FIG. 17A




FIG. 17B

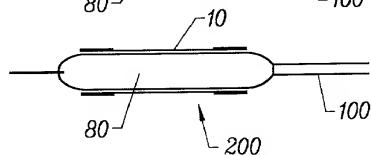


FIG. 17C

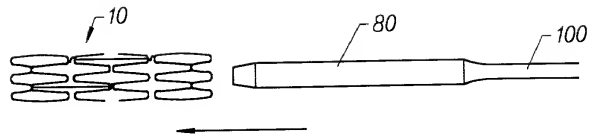


FIG. 18A

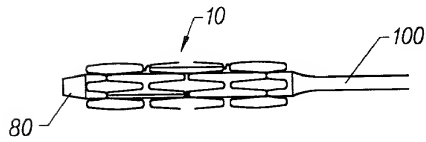


FIG. 18B

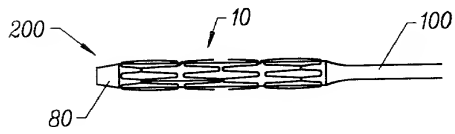


FIG. 18C

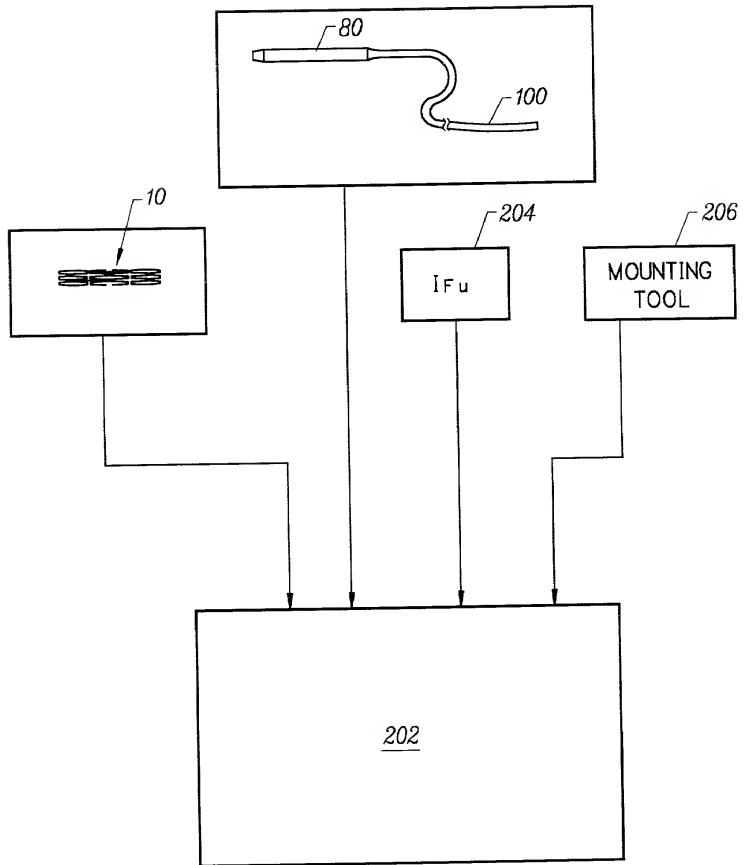


FIG. 19

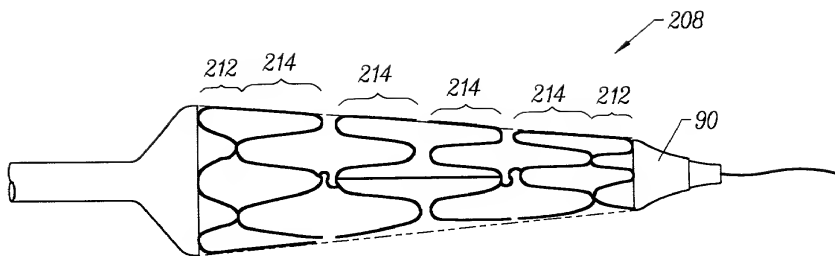


FIG. 20A




FIG. 20B




FIG. 20C




FIG. 20D




FIG. 20E




FIG. 20F

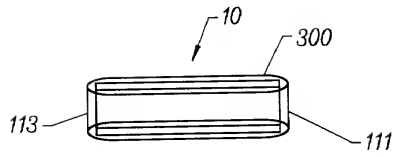


FIG. 21A

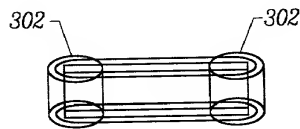


FIG. 21B




FIG. 21C




FIG. 21D




FIG. 21E

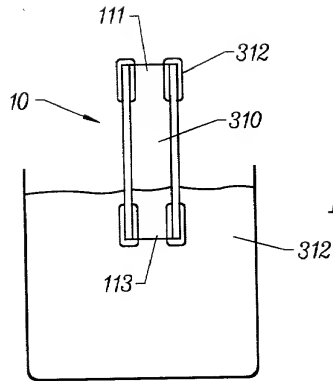


FIG. 22A

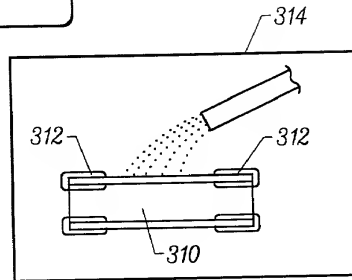


FIG. 22B




FIG. 22C

SUPPLEMENTAL DECLARATION

As a below named inventor, I declare that:

My residence, post office address and citizenship are as stated below next to my name; I believe I am the original, first and sole inventor (if only one name is listed below) or an original, first and joint inventor (if plural inventors are named below) of the subject matter which is claimed and for which a patent is sought on the invention entitled: **RADIALLY EXPANSIBLE VESSEL SCAFFOLD HAVING MODIFIED RADIOCAPACITY** the specification of which _____ is attached hereto or _____ was filed on _____ as Application No. _____ and was amended on _____ (if applicable).

I have reviewed and understand the contents of the above identified specification, including the claims, as amended by any amendment referred to above. I acknowledge the duty to disclose information which is material to patentability as defined in Title 37, Code of Federal Regulations, Section 1.56. I claim foreign priority benefits under Title 35, United States Code, Section 119 of any foreign application(s) for patent or inventor's certificate listed below and have also identified below any foreign application for patent or inventor's certificate having a filing date before that of the application on which priority is claimed.

Prior Foreign Application(s)

Country	Application No.	Date of Filing	Priority Claimed Under 35 USC 119
PCT	PCT/US96/07942	May 29, 1996	08/463,166

I hereby claim the benefit under Title 35, United States Code § 119(e) of any United States provisional application(s) listed below:

Application No.	Filing Date
60/060,938	October 23, 1997

I claim the benefit under Title 35, United States Code, Section 120 of any United States application(s) listed below and, insofar as the subject matter of each of the claims of this application is not disclosed in the prior United States application in the manner provided by the first paragraph of Title 35, United States Code, Section 112, I acknowledge the duty to disclose material information as defined in Title 37, Code of Federal Regulations, Section 1.56 which occurred between the filing date of the prior application and the national or PCT international filing date of this application:

Application No.	Date of Filing	Status
08/968,319	November 12, 1997	Pending

Full Name of Inventor 1:	Last Name: KLEIN	First Name: ENRIQUE	Middle Name or Initial: J.
Residence & Citizenship:	City: Los Altos	State/Foreign Country: California	Country of Citizenship: United States
Post Office Address:	Post Office Address: 1686 Christina Drive	City: Los Altos	State/Country: California
			Postal Code: 94024

I further declare that all statements made herein of my own knowledge are true and that all statements made on information and belief are believed to be true; and further that these statements were made with the knowledge that willful false statements and the like so made are punishable by fine or imprisonment, or both, under Section 1001 of Title 18 of the United States Code, and that such willful false statements may jeopardize the validity of the application or any patent issuing thereon.

